

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61F 2/02, A61L 27/00, A61C 8/00	A1	(11) International Publication Number: WO 95/09583 (43) International Publication Date: 13 April 1995 (13.04.95)
(21) International Application Number: PCT/SE94/00724 (22) International Filing Date: 5 August 1994 (05.08.94) (30) Priority Data: 9303206-8 1 October 1993 (01.10.93) SE (71) Applicant (for all designated States except US): LUCOCER AKTIEBOLAG [SE/SE]; Thomas Johansson, Lars Pähls väg 28, S-263 52 Höganäs (SE). (72) Inventors; and (75) Inventors/Applicants (for US only): JOHANSSON, Thomas [SE/SE]; Lars Pähls väg 28, S-263 52 Höganäs (SE). HAR- RYSSON, Ralph [SE/SE]; Professorsvägen 76A, S-951 63 Luleå (SE). HERMANSSON, Leif [SE/SE]; Bellmansgatan 34, S-754 26 Uppsala (SE). (74) Agent: HYNELL, Magnus; Hynell Patenttjänst AB, P.O. Box 2236, S-683 02 Hagfors (SE).		(81) Designated States: AM, AT, AU, BB, BG, BR, BY, CA, CH, CN, CZ, DE, DK, ES, FI, GB, GE, HU, JP, KE, KG, KP, KR, KZ, LK, LT, LU, LV, MD, MG, MN, MW, NL, NO, NZ, PL, PT, RO, RU, SD, SE, SI, SK, TJ, TT, UA, US, UZ, VN, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG), ARIPO patent (KE, MW, SD). Published <i>With international search report.</i>
(54) Title: AN IMPLANT <div data-bbox="672 1622 1627 2079" data-label="Image"> </div> (57) Abstract <p>An implant intended to be fixed through contact with new grown bone tissue, which implant at least partially consists of a dense material, which at least within a portion (1) of its surface, which surface portion shall form a contact surface for new grown bone tissue, has surface pores (2) which cover 5-40 % of said surface portion (1). Close to at least a substantial fraction of all of said surface pores there is at least one elevation (3) which extends over the implant surface which surrounds the brim (edge) of the pore.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

AN IMPLANT

TECHNICAL FIELD

5 The present invention generally relates to the field of medical applications, more particularly to the field of implantology, and concerns an implant intended to be fixed through contact with new grown bone tissue, which implant at least partly consists of a dense material having, at least within a portion of its surface, surface pores, which cover
10 5-40 % of said surface portion which shall constitute a contact surface for new grown bone tissue.

BACKGROUND ART

When using supporting implants it is important that the implant material has a high strength and that a sufficiently high resistance to shearing forces is developed between
15 the implant and new grown bone tissue; the latter feature being important for the achievement of a good retention. A high strength of implant materials can be achieved by using dense materials having an inherent high strength, such as conventional construction materials, for example stainless steel, cobalt-chromium alloys, titanium and titanium alloys, ceramic materials or polymers or materials with controlled defects, including
20 pores. For the fixation of implants it is known in the art to utilize a topographic surface or pores, wherein retention is achieved through the establishment of a good contact between the implant and new grown bone tissue.

In the Swedish patent No. 468 502, certain aspects relating in the first place to the pore
25 size distribution in porous implant materials have been disclosed. Specific and complex pore size distributions in this respect have been found possible to use for depositing bone growth promoting substances and in order to stimulate a good bone ingrowth in larger pores.

30 In a Swedish patent application No. 9200072-8 is described how the micro porosity of an implant can be utilized for the deposition of one or more bone growth promoting substances by means of carriers prior to implantation. By filling the pores to a different degree with carriers having a poor solubility, and with appropriate active agents, the formation of pores for bone ingrowth and, for release of active substances can be
35 controlled in order to achieve an optimal ingrowth.

BRIEF DISCLOSURE OF THE INVENTION

It is an object of the invention to provide an implant material having an improved retention. This is achieved, according to the invention, therein that close to at least a substantial fraction of all of said surface pores there is at least one elevation which
5 extends over the implant surface surrounding the brim of the pore. The elevation or the elevations is/are not bound to any specific topography, but preferably they should have the shape of one or more ridges which partly or completely surround the pore. In order that the desired improvement of the retention shall be achieved, at least any elevation around the pore should have an altitude amounting to at least 1 μm , suitably at least
10 5 μm , over the surrounding material surface. The height is limited in first place by conditions which have to do with production technology. Normally therefore the maximal altitude is not more than 50 μm , preferably max 20 μm .

The elevation or elevations around the surface pores, according to the invention can be
15 produced according to various techniques. In those cases when the implant material at least within the portion in question of the surface of the implant consists of a material having a good ductility, such as most metals (also alloys are included in the concept of metals), the surface pores are suitably produced through thermal etching or through
20 supersonic working. Depending on the curvature of the implant, supersonic working can be chosen, which is to be preferred on comparatively flat regions, or thermal etching for more curved parts. For the latter case, more particularly laser should be used. Preferably there is used a laser of the carbon dioxide type; YAG laser, or Excimer laser. By proper arrangement of the apparatus a desired geometry and pattern can be achieved, and by proper adjustment of the supplied power, the elevations around the pore edge can be
25 created through crater formation at the establishment of the pore in those cases when the material is sufficiently ductile. Which materials that are sufficiently ductile and how the pore formation shall be performed in order to create the said crater formation and hence the desired elevations can be determined through empirical experiments.

30 In those cases when the material within the surface portion in question has so poor ductility that any elevations can not be formed, such as craters, at the establishment of the pore by means of laser or the like, which is normally the case e.g. for ceramics, the desired elevations around the pore instead can be established by removing material in a region around the brim portion of the pore, so that the brim portion will remain as an
35 elevation over the surrounding surface.

Generally it can be said that through the invention there is achieved an improved balance between the retention and the strength of the implant material. Through optimized ingrowth of bone tissue in surface pores having beads (elevations) according to the invention, the resistance against shear forces between implant and new grown bone can
5 be increased from about 3-4 MPa for cylinders without surface pores to more than about 8 MPa for cylinders having surface pores.

Further characteristic features and aspects of the invention will be apparent from the following embodiments and from the appending claims.

10

BRIEF DESCRIPTION OF DRAWINGS

In the following description, reference will be made to the accompanying drawings, in which

- 15 Fig. 1A-C illustrate examples of some various patterns which the surface pores can form on the implant surface,
Fig. 2 shows some surface pores in Fig. 1A at a larger scale,
Fig. 3 schematically shows a section through a surface pore along a line III-III in Fig. 2, and
20 Fig. 4 shows a section through an embodiment having a theoretically ideal design with inclined surface pores.

DETAILED DESCRIPTION OF THE INVENTION

In Fig. 1A a portion of an implant surface 1 has surface pores 2 arranged in a square
25 pattern. Fig. 1B shows a portion of an implant surface 1 having surface pores 2 arranged in a hexagonal or rhombic pattern. Fig. 1C shows a portion of an implant surface 1 having surface pores 2 arranged in a spiral pattern.

In Fig. 2 there is shown a number of surface pores 2 having elevations 3 extending more
30 or less continuously around the edge of the pore. The elevations 3 have the form of crater formations, which may arise at the formation of the surface pores through working by means of laser if such parameters as supplied power, time etc. are properly set.

Fig. 3 illustrates how a pore 2 and the region adjacent to the pore may look according to
35 the invention in a typical case. In the drawing, the diameter of the pore 2 is designated D and its depth is designated d. The maximal height of the elevation or the elevations 3 over the material surface 4 surrounding the edge of the pore 2 is designated h. The ratio

between the diameter and the depth of the surface pores, D/d , and the height h of the elevation 3 are important for the retention. Thus D/d should lie within the range 0.1-10, preferably in the range 0.5-2, when the mean diameter of the surface pores 2 lies between 50-500 μm and the surface pore depth is between 10-400 μm . The height h under these conditions should be at least 1 μm , preferably at least 5 μm , while the maximal height h may be up to 50 μm , preferably max 20 μm . Preferably, the mean diameter of the surface pores 2 should be between 100-200 μm , the surface pore depth should be between 50-200 μm , and the distance between adjacent surface pores should be between 50-200 μm .

10

Fig. 4 shows surface pores 2' having inclined pore walls 5, which in combination with the elevations 3 further enhances the retention. The inclination of the pore walls 5 may amount to about 30° relative to the normal directions of the surface pore openings.

15 EXAMPLES

24 cylinders of a completely dense, i.e. without any pores interior of the surface, C P titanium having a diameter of 2.8 mm and a length of 6 mm were implanted in the femure of rabbits for 4 and 12 weeks, respectively. The rabbits were of type New Zealand White having a weight of about 4 kg. Half of the cylinders had pores, which were thermally etched by means of laser having the following apparatus parameters, wherein surface pores were achieved having a mean diameter of about 150 μm and a depth of the same order. Ridge shaped elevations were formed around the opening of the pores through the laser treatment, the ridges having a maximal height over the surrounding material surface of about 5 μm . The mean distance between the surface pores was about 120 μm .

25

Laser type

YAG

The laser beam was moved to and fro over the cylinder surface in the axial direction, the cylinder being turned between each change of movement direction

Rate of movement:

630 mm/min

Turning angle

appr 14°

Pulse frequency

30 Hz

Pulse width

0.13 ms

Lamp voltage

600 V

Pulse power

0.6 J

Beam path aperture

3.0 mm

Focal point

4.2 mm over the material surface

Prior to sterilization the implant samples were cleaned ultrasonically in HCl-solution for 1 h, whereafter the samples were stored in 1 M HCl-solution for 14 h. The samples finally were washed, firstly in di-ionized water and 70 % alcohol and secondly in destillated water. The samples were sealed in special bags and autoclaved for 20 min. In the femure (a leg) of each rabbit three holes were drilled by means of a special drilling device at a distance of about 10 mm from each other and at a distance from the growth zone in cortical bone under a heavy saline flow in order to promote efficient cooling. A low drilling pressure was applied. The drilling produced holes having appr 0.1 mm play for the cylinder samples. After the period of implantation, the animals were put to death by an overdose of Mebumal, and were prepared for so called push-out tests and for histological evaluation.

A 10 mm long bone section with the implant in the centre thereof was prepared from the femure. The bone sections were cut longitudinally in order to make available the part of the implant facing the bone marrow. The prepared bone was kept in 0.9 % NaCl solution without any fixation. Bone with cylinder was placed in a push-out fixture by means of a dental cement. The maximal force required for loosening the implant from the bone was detected by means of a universal instrument for measurement of strength (Alwetron) having a loading rate of 0.5 mm/min. The shear force between implant and bone was calculated through measured power divided by the present contact surface between bone and implant. The results are given in Table 1.

Table 1 - Shear power between implant and bone

U = without surface pores M = with surface pores

Animal No	Implant 1 MPa	Implant 2 MPa	Implant 3 MPa	Animal No	Implant 1 MPa	Implant 2 MPa	Implant 3 MPa
	6 weeks				12 weeks		
1	U 2.1	M 8.3	M 11.4	5	U 3.7	M 15.8	M 17.2
2	U 1.6	M 7.9	M 8.9	6	U 4.3	M 14.9	M 20.1
3	U 1.9	U 2.3	M 7.7	7	U 3.3	U 4.7	M 18.8
4	U 2.2	U 0.8	M 10.1	8	U 4.2	U 3.9	M 16.4

CLAIMS

1. An implant intended to be fixed through contact with new grown bone tissue, which implant at least partly consists of a dense material having, at least within a portion (1) of its surface, surface pores (2), which cover 5-40 % of said surface portion (1), which shall
5 constitute a contact surface for new grown bone tissue, c h a r a c t e r i z e d in that close to at least a substantial fraction of all of said surface pores there is at least one elevation (3) which extends over the implant surface surrounding the brim (edge) of the pore.
- 10 2. An implant according to claim 1, wherein the elevation or the elevations consist of a ridge or ridges completely or partially surrounding the pore.
3. An implant according to claim 1 or 2, wherein the maximal height (h) of the elevation over the material surface (4) amounts to at least 1 μm and maximal 50 μm .
15 4. An implant according to claim 3, wherein the maximal height of the elevation of the over the implant surface (4) amounts to at least 5 μm but not to more than 20 μm .
5. An implant according to any of claims 1-4, wherein at least that part of the implant
20 surface which comprises the portion (1) having said surface pores consists of a metal, of a polymeric, or of a composite material substantially consisting of a metal or of a polymer.
6. An implant according to any of claims 1-4, wherein at least that part of the implant
25 which comprises the portion (1) having said surface pores consists of a ceramic or of a composite material substantially consisting of a ceramic material.
7. An implant according to any of claims 1-6, wherein the surface pores as well as the
30 elevations which completely or partly surround the surface pores are produced through laser treatment of the implant material.

1 / 2

A.


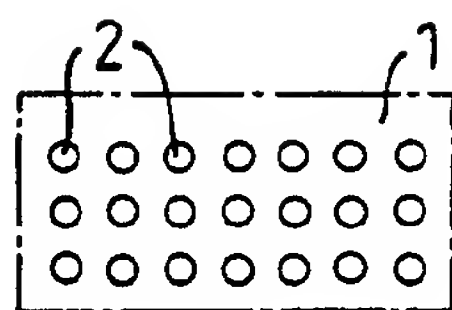


Fig. 1

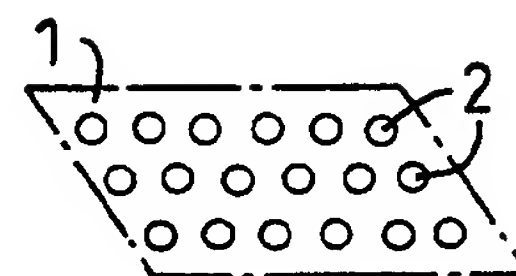

B.

C.

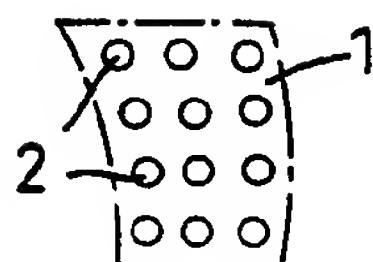


Fig. 2

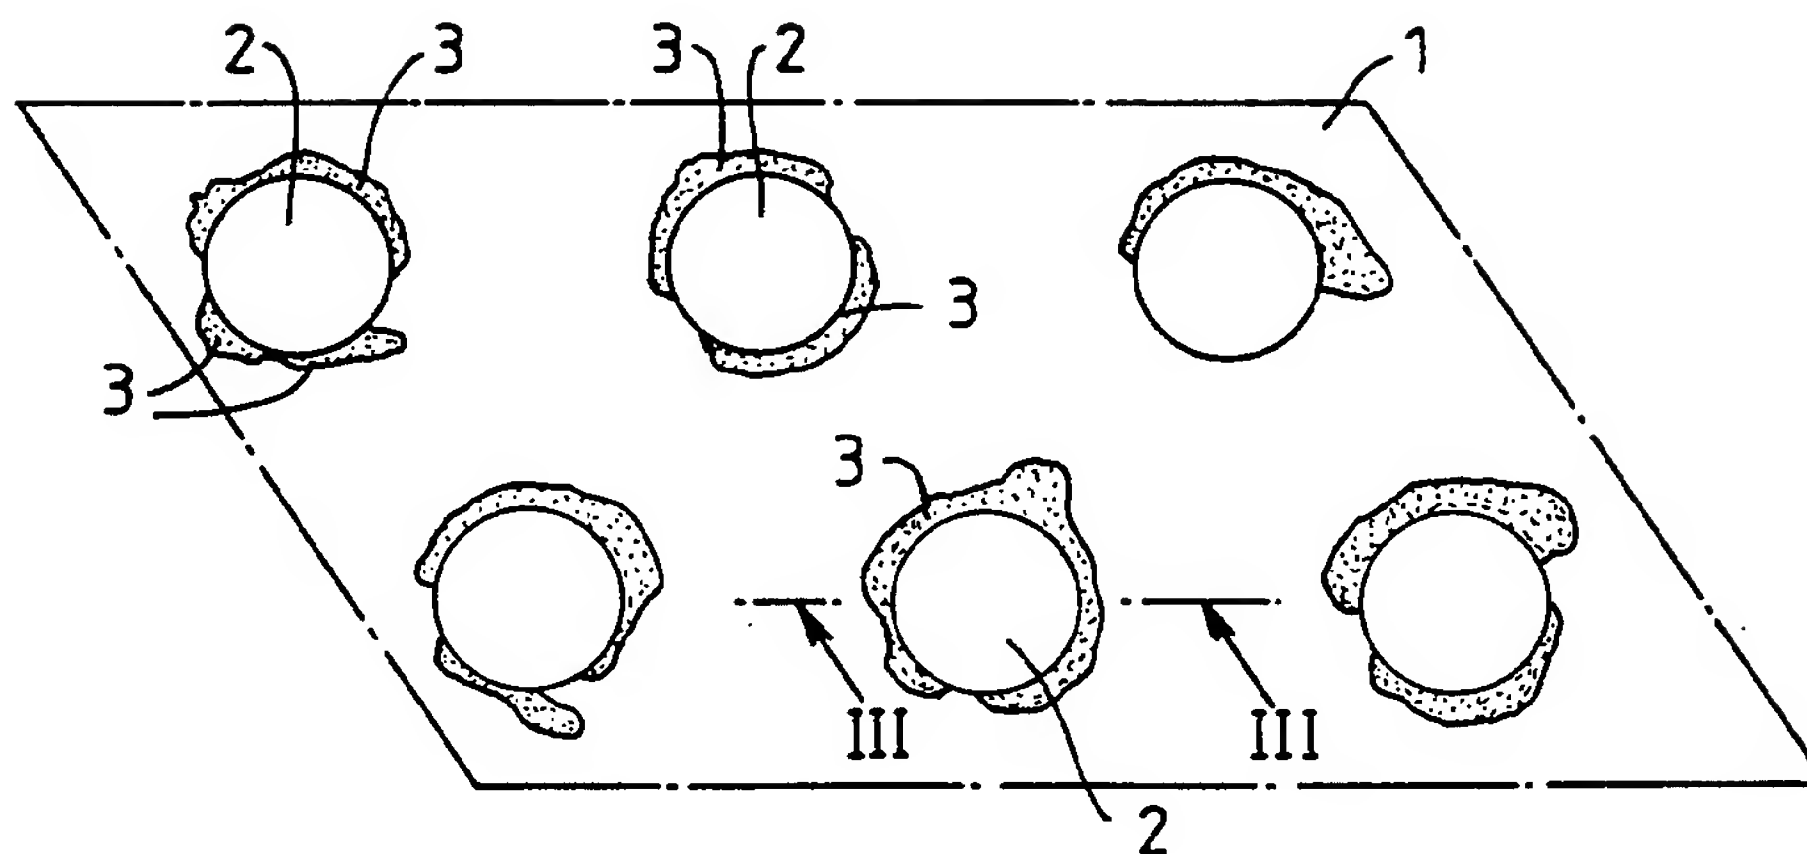


Fig. 3


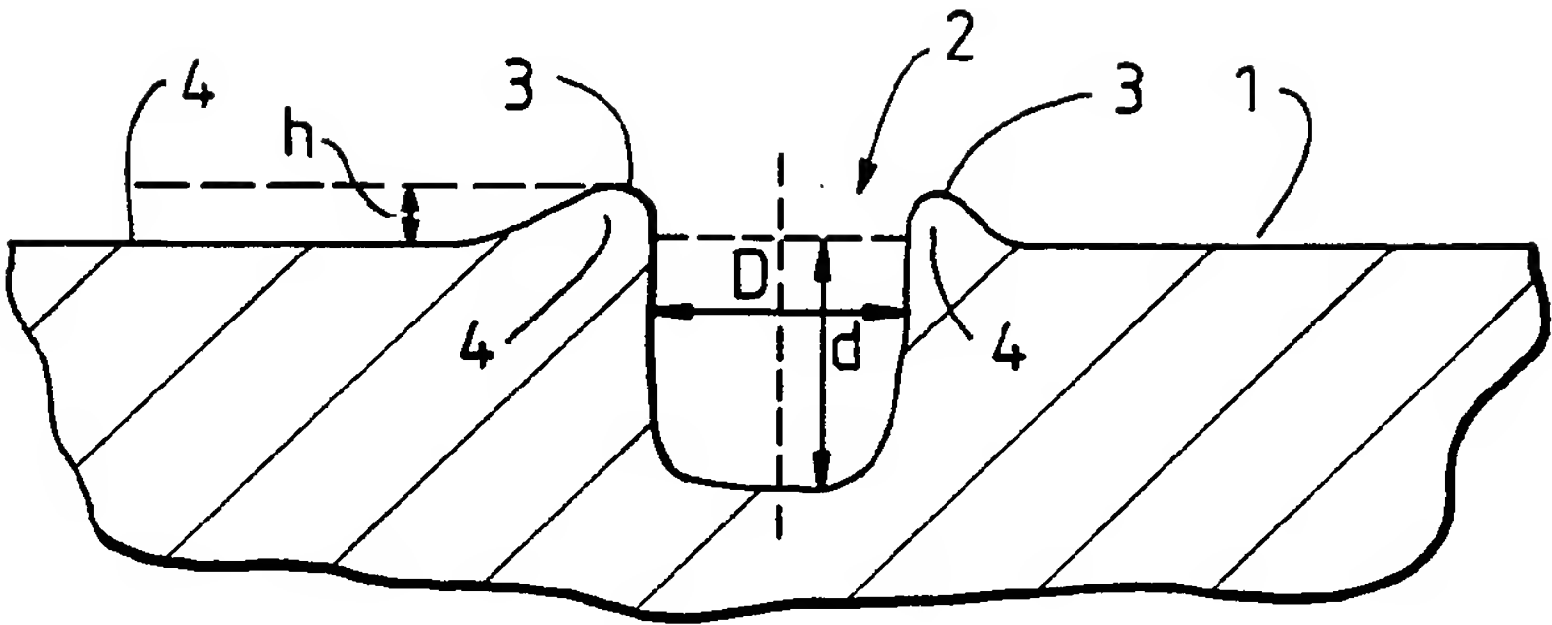


Fig. 4

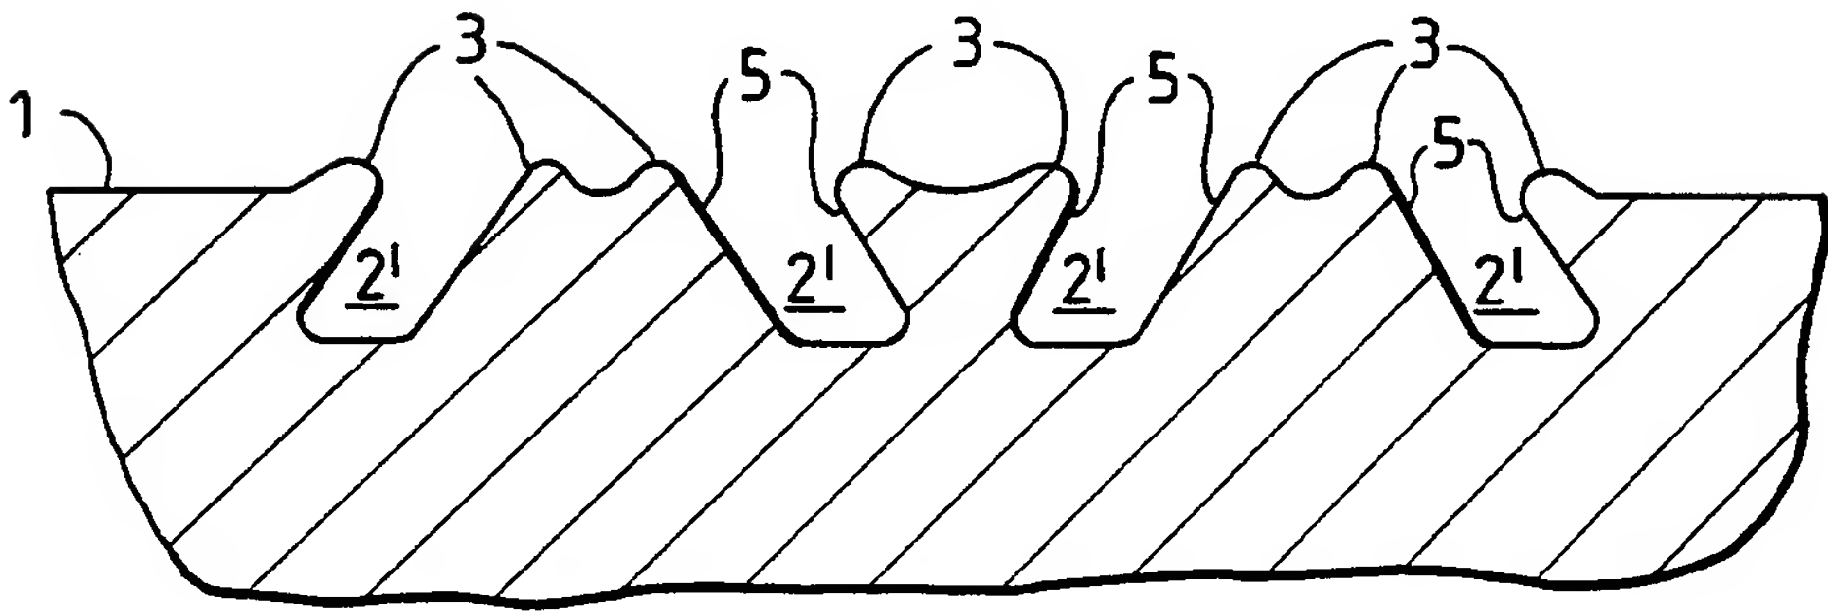

INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 94/00724

A. CLASSIFICATION OF SUBJECT MATTER

IPC6: A61F 2/02, A61L 27/00, A61C 8/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC6: A61C, A61F, A61L

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US, A, 5222983 (HERMANN-JOSEPH SCHMITZ ET AL.), 29 June 1993 (29.06.93), column 3, line 5 - line 12, figure 2	1 - 4
Y	--	5-7
Y	WO, A1, 9221302 (LUCOCER AKTIEBOLAG), 10 December 1992 (10.12.92), claims 1-9	5-7
A	WO, A1, 9313815 (LUCOCER AKTIEBOLAG), 22 July 1993 (22.07.93), claims 1-7	1,5-6

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

17 January 1995

Date of mailing of the international search report

20 -01- 1995

Name and mailing address of the ISA/
Swedish Patent Office
Box 5055, S-102 42 STOCKHOLM
Facsimile No. +46 8 666 02 86

Authorized officer

Leif Brander

Telephone No. +46 8 782 25 00

INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 94/00724

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US, A, 4865603 (DOUGLAS G. NOILES), 12 Sept 1989 (12.09.89) ----- -----	1,5

INTERNATIONAL SEARCH REPORT

Information on patent family members

31/12/94

International application No.

PCT/SE 94/00724

Patent document cited in search report		Publication date	Patent family member(s)		Publication date
US-A-	5222983	29/06/93	AT-T-	115386	15/12/94
			DE-U-	9013067	06/02/92
			EP-A,B-	0475358	18/03/92
			JP-A-	4246360	02/09/92
			DE-U-	9100075	30/04/92

WO-A1-	9221302	10/12/92	AU-A-	1908192	08/01/93
			AU-A-	3963793	30/12/93
			SE-B,C-	468502	01/02/93
			SE-A-	9101677	04/12/92

WO-A1-	9313815	22/07/93	AU-A-	3269993	03/08/93
			CZ-A-	9301643	16/02/94
			EP-A-	0623031	09/11/94
			SE-B,C-	469653	16/08/93
			SE-A-	9200072	14/07/93

US-A-	4865603	12/09/89	NONE		
